

Catheterization/Enema Simulator

Basic high quality trainings in male and female: urethral catheterization, perineal care and enema.

Soft and anatomically correct genitals and realistic feeling of catheter insertion. Organ unit can be used independently without the lumbar torso, allowing training with SPs or full body manikins in clinical settings. The newly devised modular system realize easy set-up, cleaning and maintenance, saving time and cost for training providers.

MW2A Male Catheterization/Enema Simulator



MW2B Female Catheterization/Enema Simulator



Training Skills

- Intermittent catheterization
- Perineal care
- Location of urethral meatus
- Indwelling catheterization
- Enema
- Cleansing
- Catheter insertion and placement
- Withdrawal of catheter
- Manual bladder compression

Features



Soft genitals allows realistic cleansing and procedures like

- parting the labia
- holding the penis perpendicular to body
- retracting the foreskin

Successful catheter insertion is confirmed by urine (water) out ow.

Manual bladder compression is possible.

Enema training in lateral position.

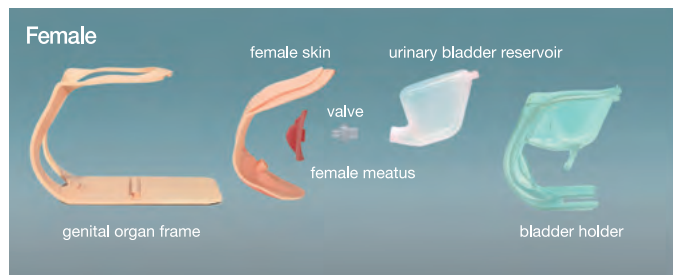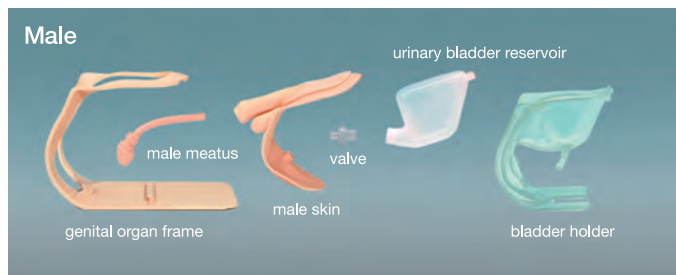

Simple and Easy to Upkeep

Organ parts can easily be disassembled and reassembled.

KYOTO KAGAKU

15 Kitaneokoya-cho, Fushimi-ku, Kyoto, 612-8388, JAPAN

Tel: +81-75-605-2510 Fax: +81-75-605-2519

www.kyotokagaku.com rw-kyoto@kyotokagaku.co.jp

Soft and Anatomically Correct Genital



Male: Retractable foreskin.
Catheters can be inserted only with the correct perpendicular penis position.
Anatomically correct length of urethra.



Female: Soft, separable labia.
Anatomically correct length of urethra.

Catheter Insertion and Placement



Realistic feeling and resistance of catheter insertion.
Successful insertion is confirmed by urine (water) outflow.
Indwelling (Foley) catheter can be anchored with balloon.
Passing catheter can be observed through transparent wall of the bladder reservoir.

Training With SP




Organ unit can be used separately, allowing training with SPs or full body manikins in clinical settings.

Manual Bladder Compression



Manual bladder compression to check or release residual urine.

Enema Training

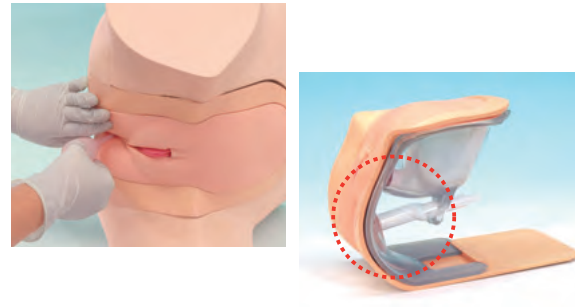

The lower torso can be placed in lateral position for enema training. To learn safe insertion of the enema tube, the perineal flexure is represented.

MW2A Male Catheterization/Enema Simulator

MW2B Female Catheterization/Enema Simulator



Male



Female

Each set includes:

- 1 lower torso manikin
- 1 genital organ unit
- 3 valves
(one is incorporated in the assembled unit.)
- 1 irrigation bottle
- 1 rectum tube
- 3 irrigation drainage tubes
- 1 lubricant
- 1 instruction manual

Manikin size: 34 x 33 x 24H cm

*recommended catheter size
16Fr. and 14Fr. Foley catheters for male and female respectively.

Specifications are subject to change.

Replacement parts

- 11381-300 replacement valve for MW2A/B (a set of 6)
- 11381-400 replacement male skin
- 11381-500 replacement male meatus (a set of 2)
- 11381-600 replacement female skin
- 11381-700 replacement female meatus (a set of 2)



11381-300



11381-400



11381-500



11381-600



11381-700