



Caution


Do not mark on the product and its components with a pen or allow printed materials to come in contact with the surface. Ink marks cannot be removed.

MW50

Strap-on Venipuncture Trainer II

Instruction Manual

Content

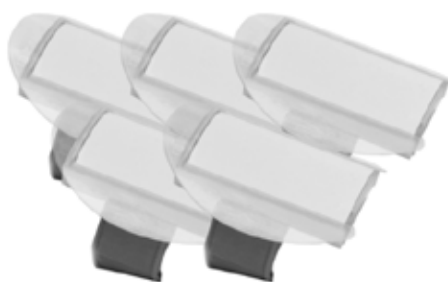

- Before you start
 - Features P.10
 - Set includes P.11
- Preparation
 - Preparation for training P.12
 - Filling Water P.13
 - Fitting the pad P.14
- Training
 - Training procedure and notes P.15
- After training P.16
- Replacing consumables P.17

Before you

The simulator is designed for training in IV injection and blood collection. Do not use for improper purpose. Please read the instruction carefully before use.

Features

- Pads made from a new material with significantly improved puncture durability.
- Adopts a simple setting method to set the pad in the holder.
- Attaching it to SP (standardized patient) or the arm of a full-body model allows for realistic intravenous injection training.



DOs and DON'Ts

DOs

The materials for the models are special compositions of soft and hard resin.

Please handle them with the utmost care at all times. Store the training set at room temperature, away from heat, moisture and direct sunlight.


DON'Ts

Never wipe the simulator with thinner or organic solvent.

Don't mark on the simulator with pen or leave any printed materials in contact with their surface. Ink marks cannot be wiped out.

Set includes

Before your first using, ensure that all components listed below are included.

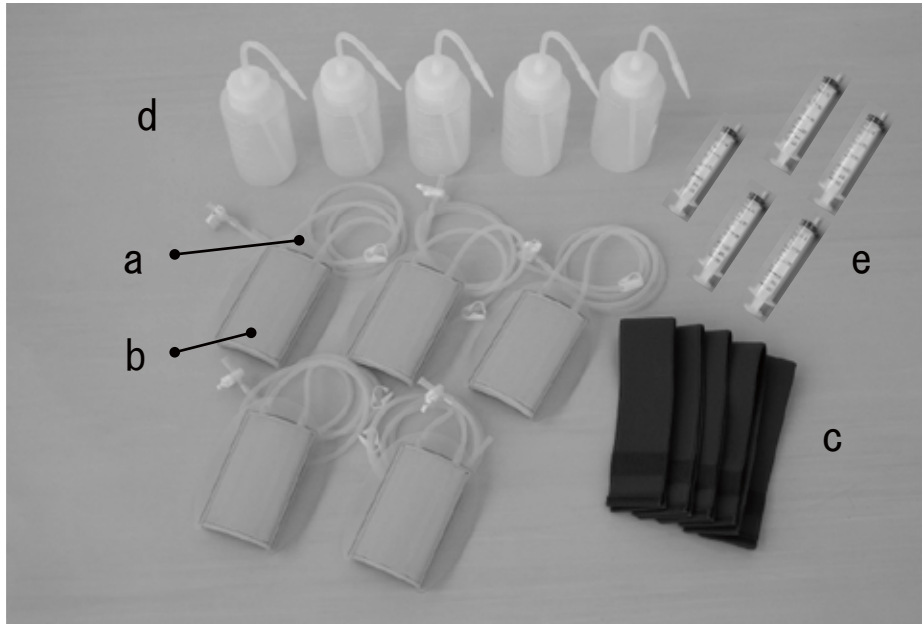

- a. Supporting frame ····· 5
 - b. Puncture Pad ····· 5
 - c. Strap belt ····· 5
 - d. Water bottle ····· 5
 - e. Syringe ····· 5
- And Instruction manual

In addition to the included components, please prepare a container for draining water.

① Advanced Preparation


1. Preparation of simulated blood

Pour about 300 cc water or simulated blood into the water bottle.



2. Unlock the pinchcock

Unlock the pinchcock for the water supply tube.

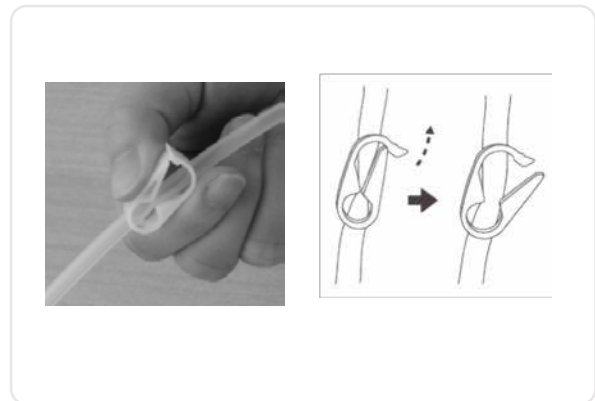

3. Connection of the water supply tube


Insert tip of the water supply tube (approx. 1cm) to the spout of the water bottle.



① Filling

1. Connection of the drain tube

Insert the three way cock connected to the tips of the drain tube to the tips of the syringe.

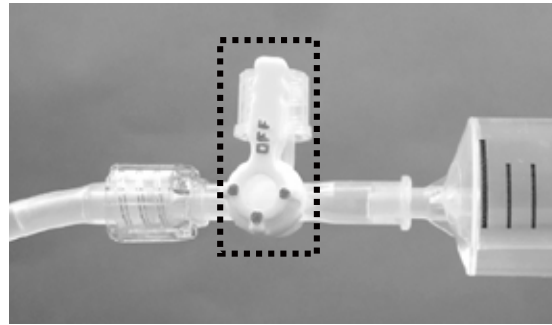


2. Water supply

Pulling plunger of the syringe, fill the tube with water.




Caution

.....
Be sure to draw the piston of the syringe.
If you push the piston forcibly, increasing the internal pressure in the tube, or pull the syringe too quickly, it may cause damage to the pad or water leakage.

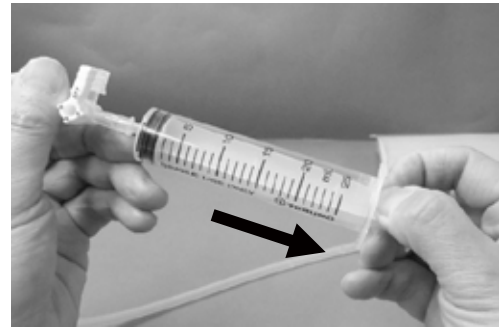

3. Check filling and close three way cock.

Check filling the syringe with water, then stop pulling the plunger and close the cock as shown in the picture.

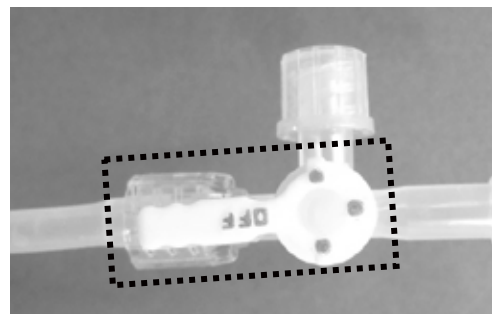

4. Remove the syringe.

Remove the syringe.

*Before removing, check that the three way cock is closed.



② Attaching the pad

1. Wrap the strap belt

Wrap the strap belt around the site on the arm/hand for training.



2. Fix the pad holder to the strap belt

Fix the pad to the strap belt.

The back of the pad holder has the Velcro. So just only putting the pad holder on the strap belt, the pad is fixed at any site on the belt.



Training procedure


1. Training

During the practice session, keep the bottle at the same height with the trainer.

The two lines of puncture sites are on the pad as shown in the picture to the right.

Please note

When you do training with the simulated blood, be careful not to drop the liquid on the cloth. The liquid dropped on the cloth may be irremovable stain.

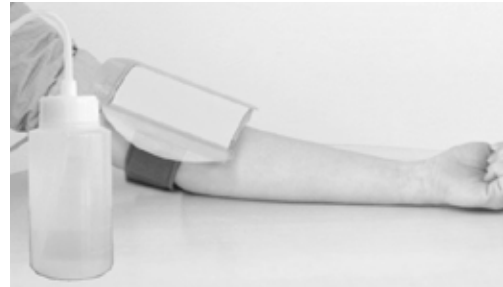

2. Refilling Water

When the water in the water bottle is reduced, remove the trainer from the arm, and replenish water following the procedures in P3.




After training

After training session, discharge water from the trainer and tubes following the procedure below.


1. Disconnect the water supply tube.

After lock the pinchcock, disconnect the water supply tube from the spout of the water bottle.

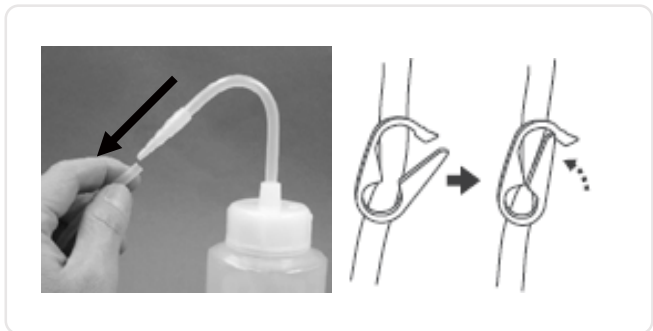

2. Disconnect the drain tube.


Close the three way cock as shown in the right picture, then disconnect the three way cock from the syringe.

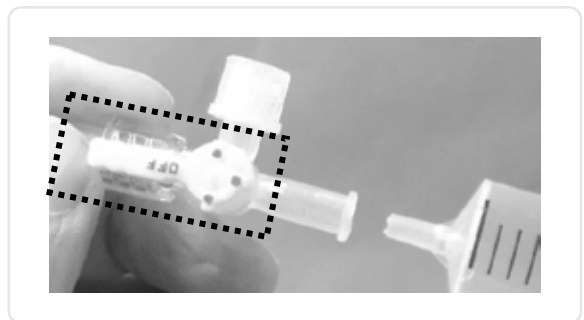

3. Discharge water


Place both water supply and drain tubes into container, then open the three way cock as shown in the right picture.

When the pad is lifted, water in the pad is discharged.

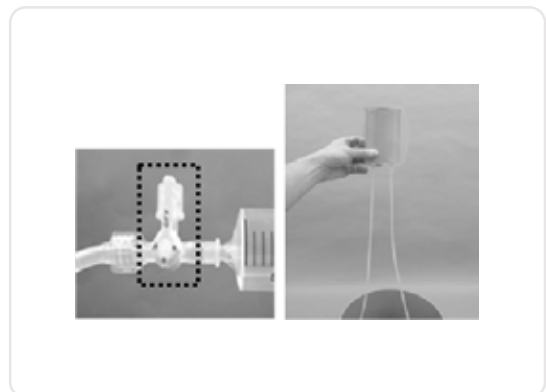

**Please
note**

Do not remove the soft part as show in the right picture. Removing may cause the water leak.

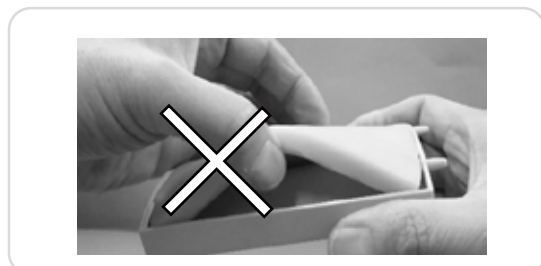


4. Clean the pad



When cleaning the pad, wipe the pad with water, neutral detergent or alcohol.

Replacing consumables

1. Drain all water from the old pad and disconnect both the water supply tube and drainage tube. Then, pull out the pad from the frame.

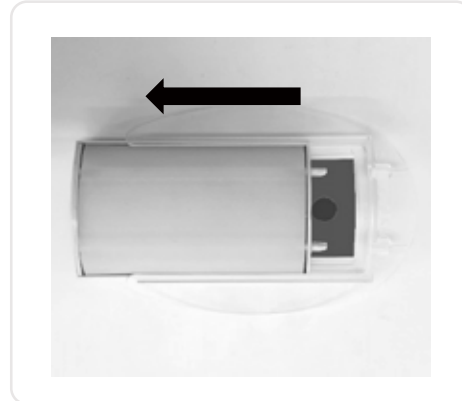

2. Slide a new puncture pad into the back of the frame.

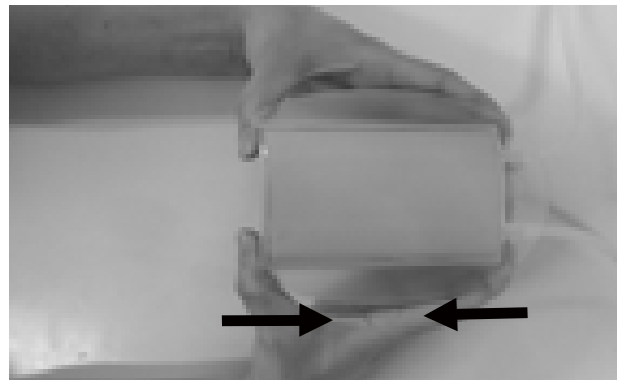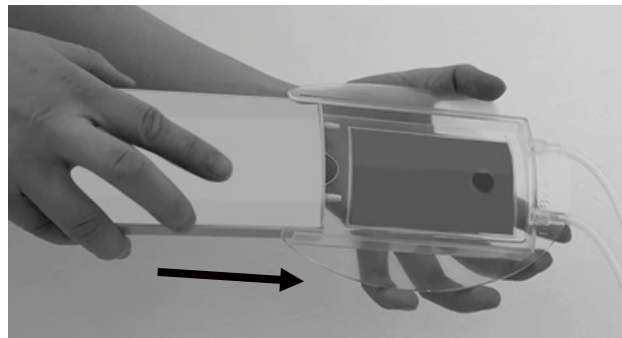

Please note

Press the pad firmly into the holder. Insufficient attaching may cause the leak of water from the connection of pad and pad holder as shown in the below picture.



Consumable

Code	Name
11431-010	Puncture pad (Set of 5)




Puncture pad (Set of 5)

Optional parts

Code	Name
11430-010	Arm Vessels Anatomy Sleevelet
11388-400	Cotton Swab for Coloring (Red) 10 pcs



Arm Vessels Anatomy Sleevelet

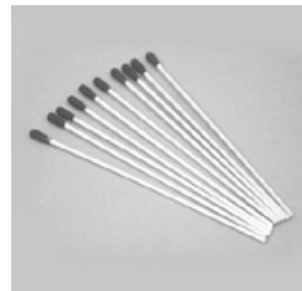

Cotton Swab for Coloring (Red) 10 pcs



注意

モデル表面に印刷物などが直接触れないようにしてください。
樹脂にインクが吸収されて消えなくなります。



Caution

Do not let ink from pens, newspapers, product manual or other sources contact the manikin. Ink marks on the manikin will be irremovable.

- 本製品についてのお問い合わせや不具合等ございましたら、お手数ですがお買い上げの販売店、もしくは下記（株）京都科学まで御連絡ください。
- For inquiries and service, please contact your distributor or KYOTO KAGAKU CO., LTD.



株式
会社

京都科学

URL・<http://www.kyotokagaku.com> e-mail・rw-kyoto@kyotokagaku.co.jp

■ 本社・工場

〒612-8388 京都市伏見区北寝小屋町15番地
TEL: 075-605-2510 (直通)
FAX: 075-605-2519

■ 東京支店

〒113-0033 東京都文京区本郷三丁目26番6号
NREG本郷三丁目ビル2階
TEL: 03-3817-8071 (直通)
FAX: 03-3817-8075

■ Main Office and Factory (World Wide)



KYOTO KAGAKU co.,LTD

WEB・www.kyotogagaku.com

E-MAIL・rw-kyoto@kyotokagaku.co.jp

15 kitanechoya-cho Fushimi-ku Kyoto 612-8388, Japan
TEL: +81-75-605-2510
FAX: +81-75-605-2519

■ North and South American regions:



KKAmerica

Kyoto Kagaku America Inc.

WEB・www.kkamerica-inc.com

E-MAIL・info@kkamerica-inc.com

3109 Lomita Boulevard, Torrance, CA 90505-5108, USA
TEL: +1-310-325-8860
(Toll-free in North America: 877-648-8195)
FAX: +1-310-325-8867

本書の内容は、予告なしに変更することがあります。本書の内容の一部もしくは全部を当社に無断で複写・転載することを禁じます。

本書の内容に、万一不審な点や誤りなど、お気づきの点がございましたら、当社もしくは販売店にご連絡ください。

The contents of the instruction manual are subject to change without prior notice.

No part of this instruction manual may be reproduced or transmitted in any form without permission from the manufacturer.

Please contact manufacturer for extra copies of this manual which may contain important updates and revisions.

Please contact manufacturer with any discrepancies in this manual or product feedback. Your cooperation is greatly appreciated.