▲ Caution

Do not mark on the model and its components with a pen or leave printed materials in contact with the model surface. Ink marks on the model are not removable.



MW57 Pediatric Lung Sound Auscultation Trainer

 Product Supervision Yuki Okamatsu, MD Director of Pediatric department, Aso lizuka Hospital



Table of contents



Introduction

Before use / Features / Training skills • • • • •	P.1
DOs and DON'Ts \cdot · · · · · · · · · · · · · · · · · · ·	P.2-3
Set includes • • • • • • • • • • • • • • • • • • •	P.4
Part names and functions • • • • • • • • •	P.5

Preparation

Assembly •	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	P.6-7
	+	he		ni	t <	er	าล	ra	tel	v	•	•	•						P۵

Training

Auscultation sites/ Cases • • • • • • • • • • • • • • • • • •	P.9
Classification of lung sounds • • • • • • • • • •	P.10
Turning on the unit $\cdot \cdot \cdot$	P.11
Error indicator system • • • • • • • • • • • • • • • • • • •	P.12
Starting up the software • • • • • • • • • • • • • • • • • • •	
Operation screen • • • • • • • • • • • • • • • • • •	
Multi-unit operation • • • • • • • • • • • • • • • • • • •	P.16

After Training

Exiting the software •	•	•	•	•	٠	•	•	•	٠	٠	•	•	•	P.17
------------------------	---	---	---	---	---	---	---	---	---	---	---	---	---	------

Trouble Shooting

Trouble shooting list • • • • • • • • • • • • • • • • • • •	P.18
Unable to start the main unit • • • • • • • • •	P.19
Unable to select the unit • • • • • • • • • • • • • • • • • • •	P.20

- Error occurs during the session • • • P.21
- How to switch to LAN connection mode • • P.22



Before use Features

Before use

MW57 Pediatric Lung Sound Auscultation Simulator is designed for medical education training. Please do not use the product for other purposes. Any other use not in accordance with the instructions on this manual as well as on the help menu in the system is strongly discouraged. The manufacturer holds no responsibility for any accidents or damages resulting from such use.

For questions regarding this simulator, please contact our distributor in your area or Kyoto Kagaku. The contact information can be found on the back cover of this manual.

Features

- Sounds are recorded from actual patients and are reproduced by using a high quality sound system.
- An actual stethoscope can be used.
- · Sounds are distributed from five anterior and six posterior sites simultaneously.
- 20 lung sound cases: with and without heart sounds.
- Up to five simulators can be controlled by one wireless tablet.
- The error indicator system facilitates maintenance of the system to keep "Pediatric LSAT" in its best condition.

Skills

Pediatric lung sounds auscultation

Introduction

Supply voltage: AC100-240V 50/60Hz 450VA Altitude: 2.000 meters above sea-level Environmental conditions: 5°C.to 40°C. Relative humidity: Less than 80%(no condensation) Overvoltage Category: 2

Pollution Degree: 2

Power cord supply: Do not use power supply cords other than the one included in the original set.

Clean-up: Clean the simulator with water or mild detergent. Clean the manikin with water or mild detergent and coat with baby powder. Be careful not to apply water or detergent on the internal machinery.

Introduction

DOs and DON'Ts

DOs and DON'Ts

DOs

Operate the system under the designated circumstances

Power input: AC100V $\sim\!240V$ plus or minus 10%, 50Hz/60Hz Temperature range: between 0 degrees C and 40 degrees C (no congelation)

Relative humidity; between 0%to 80% (no condensation)

*Connecting to power source outside of the designated range may lead to fire.

Safe disposition

To avoid short circuit, do not run the simulator set above a power receptacle.

•Handle the power plug and cord observing following precautions

- 1. Clean the head of the plug periodically.
- 2. Plug in the plug to the outlet firmly to the end.
- 3. Always hold the plug when unplugging. Do not pull the cable.
- 4. Do not force to bend, twist the cable and avoid scratching or cutting on it.
- 5. Unplug the power cord when the simulator is not in use.

6. Remove any dust that has accumulated on the power plug and insert the plug completely into the power socket.

Failing to follow the above precautions can result in damage in the plug and the cable, constituting risk of fire or shock.

When the electric parts get warm or produce smoke, immediately turn off the power and unplug from the power source

Risk of fire. Contact your distributor or the manufacturer for repair.

Handle with care

The materials for the models are special compositions of soft resin. Please handle them with utmost care at all times.

Clean the manikin with water or mild detergent and coat with baby powder. Be careful not to apply water or detergent on the internal machinery.

Transport the simulator with caution. Hold the simulator by the handles when transporting. Do not hold the simulator by the torso manikin.

Storage

Store the simulator at room temperature, away from heat, moisture and direct sunlight.

Storage under the temperature above 50 degrees C may reduce the performance quality of the simulator.

Ouse the simulator in quiet environment

•Follow the instructed shutting down procedures

Shut down the computer first. Do not turn off the power or unplug the power cord without shutting down the program. Misuse may lead to damages.

DON'Ts

Do not disassemble or open electric or precision components

Do not remove or alter cable connections in the inner machinery. Connection cables and their settings have been preset; changes to the set up may lead to malfunctions or damages to the simulator. Also, do not open up or disassemble the housing for electric parts or precision components.

Refrain from opening up any lids, caps or covers for such area, and never run the system while any of such covers are open.

*Never disassemble the electric components, power plug and cable as it may create a risk of fire, shock or injury. Contact your distributor or the manufacturer for repair.

•Never wipe the product and components with thinner or organic solvent

Ink marks on the soft surface won't be

removable Don't mark on the product and components with pen or leave any printed materials in contact with their surface.

Do not give shocks

The electric components are precision instruments. Strong shocks or continuous vibration may cause breakages of its internal structure.

•Do not run the system continuously over

2 hours

Take at least 30 minutes shutdown, turning off the power, every 2 hours.

Do not wet the electric components

Do not pour or spill water or liquid detergent over the electric components, power cable and power plug. Running the system while the electric components are wet may create a shock hazard or a risk of fire.

•Do not handle the power plug with wet hands

Risk of shock.

No fire

Do not put the product close to fire. It may lead to discoloration or deformation of the product as well as short circuit, creating a risk of fire.

•Do not install other software onto the computer


It may lead to system malfunctions.

Discoloration of the surface may occur after a long period of time. Discoloration does not affect the function and performance of the simulator.

Set includes

Set includes

Before you first use "Pediatric LSAT", ensure all components listed below are included in the unit.

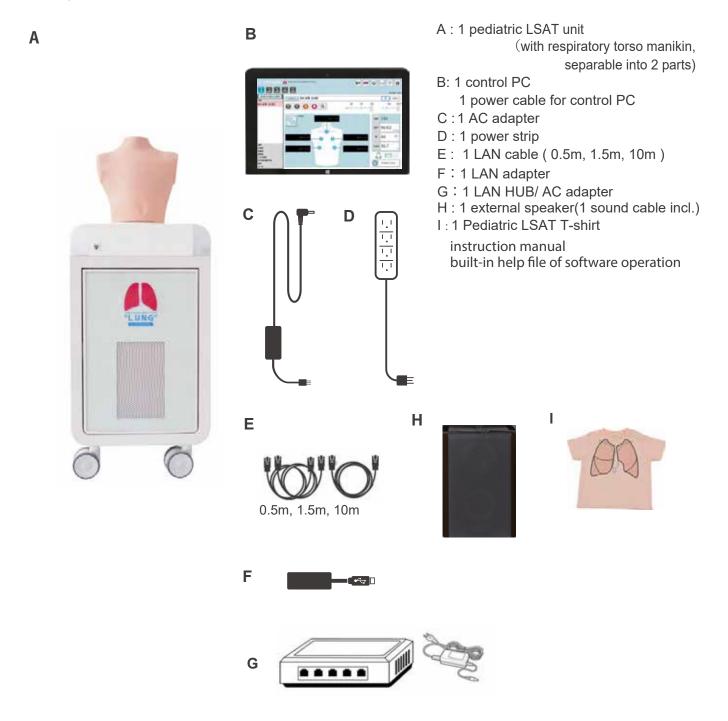


^{*}Type and specs are subject to change.

Introduction

Parts names and functions

Unit

NOTES

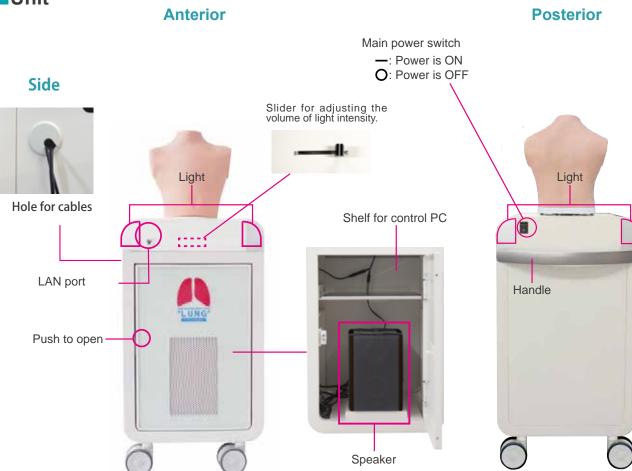

Control PC Touch-panel monitor Power button 21 61 AN 28 1081 (T) 38% 0000B 2 - 1 -Check the enclosed separate HR 140 manual about how to use of BP 96/62 the control PC. 8 40 Power supply port -36.7 £ 🗆 *Connect the power cable to the O Paistie port to charge the control PC. . *Type and specs are subject to change.

Posterior and anterior sound can be played simultaneously.


1


3

4

Installation of external speaker

) Press the red circled area to open. Find two fixing belts at the floor of the housing and unbuckle them.



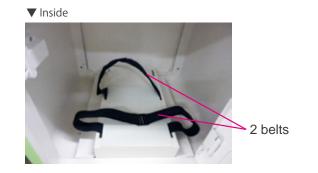

Power cable

Remove the cap of the hole for cables in the side panel.
 Pass the cable of AC adapter through the hole then connect it to the power cable at the upper area of the housing.
 Hole for cables






AC adapter

Cap

Connect the speaker and the sound output by the

sound cables for the speaker. The jacks of the speaker are at its back. Pass the power cable of the speaker through the hole on the side panel and then connect it to the power strip.

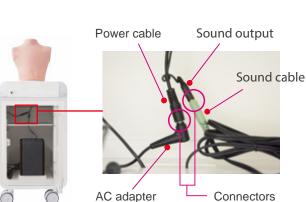

Sound cable Power cable

Speaker


Sound output

Adjust the sound volume to the position indicated by arrow marks.



*The position of the arrow marks may vary depending on the unit.



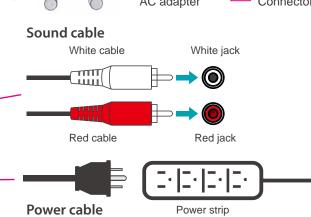

Preparation

Assembly

5

Buckle and pull the belt tightly to secure the speaker in place.







Ensure that the antennas are connected firmly to the main unit before use, or they might come off accidentally.

Introduction

How to use the unit separately

2

POINT


The torso manikin is able to be separated.

1


marked with red circles.

Detach connection cables





To separate : Push **B** button To attach : Push A knob






Hold the simulator by the handles at both sides when separating.

4

Connect unit to AC adapter to start using.







Keep the unit attached to base unless used separately.


Auscultation sites Cases

Auscultation sites



Anterior

4. lower left lung field 5. lower right lung field



Posterior

- 0. upper left lung field 1. upper right lung field 2. middle right lung field 3. middle left lung field

- 4. lower left lung field
- 5. lower right lung field


Cases 20 lung sound cases

1. trachea

2. upper right lung field 3. upper left lung field

Normal	Abnormal
A01 standard	B01 weak: left lower area B03 weak: left whole area B05 weak: right lower area B07 weak: right whole area
Coarse Crackles	Fine Crackles
C01 right lower area C03 both lower area C05 left lower area C07 both upper area C09 whole area C11 right upper area	D01 both lower area D03 whole area
Wheezes	Rhonchi
E01 trachea and upper area E03 whole area	F01 trachea and upper area F03 whole area
Miscellaneous continuous sounds	Miscellaneous (combined cases)
G01 stridors	H01 coarse crackles and rhonchi H03 fine crackles and wheezes

Classification of lung sounds

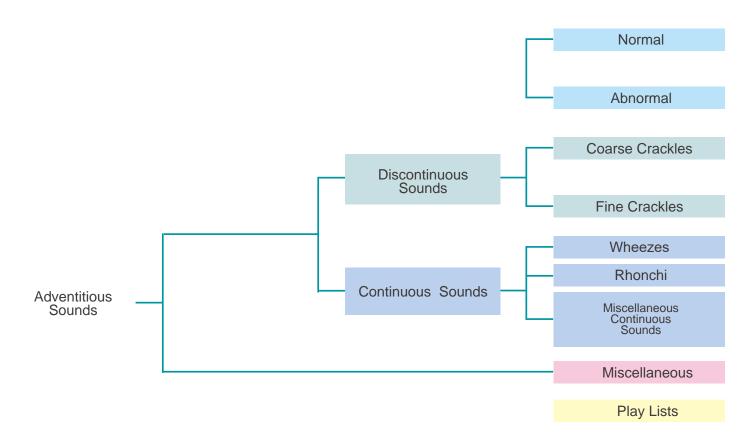

Classification of lung sounds	The American Thoracic Society developed a rational and clinically useful classification based on acoustic analysis of tape recordings and introduced the nomenclature. With this approach, lung sounds are categorized as continuous (wheezes, rhonchi, or stridor) or discontinuous (crackles). Crackles are further identified as fine or coarse. The terms "lung sounds" and "breath sounds" are usually used synonymously.
Adventitious sounds	Adventitious lung sounds are superimposed on the breath sounds in certain circumstances and usually indicate disease. They are categorized as continuous (wheezes, rhonchi, or stridor) or discontinuous (crackles). Crackles are further identified as fine or coarse.
Discontinuous sounds	Discontinuous adventitious lung sounds are intermittent, nonmusical, and brief (duration of less than 25ms) noises. They may be fine crackles (relatively high-pitched sounds usually heard at the end of inspiration as air enters the acinar unit) or coarse crackles (the low-pitched, bubbling sounds that result from the accumulation of secretions in larger bronchi and trachea).
Continuous sounds	Continuous adventitious lung sounds are usually louder than the underlying breath sounds. The word "continuous" in this context implies duration of more than 250ms rather than meaning a sound that continues throughout the respiratory cycle. Continuous sounds may be wheezes, rhonchi, or stridor.




Turning on the unit



When starting up the system follow the sequence of actions instructed below so that the wireless connection works correctly. The unit may not work correctly when turned on with aa-^!^} of order.

) Connect the power cable to the outlet.

) Turn on the control system's main power.

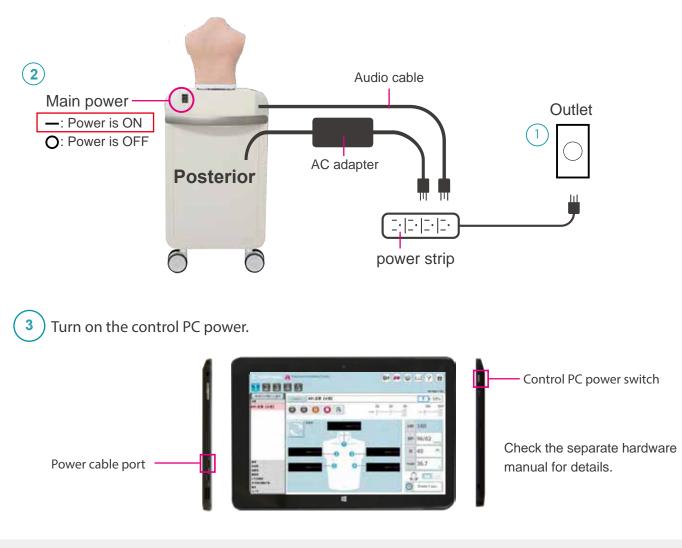

NOTES

Before starting, be sure to charge the battery of the control PC. In case that the battery is low or empty, charge it by connecting the power cable of the control PC. The system can be used with the control PC being connected to the power.


Error indicator system



2

Error indicator system

When activating Simulator "Pediatric LSAT", errors are checked automatically.

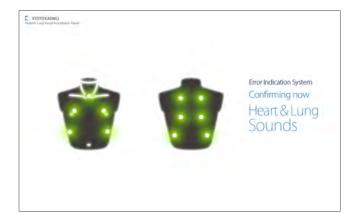



Error indication results


After the error indication , the following screen shows up. Make sure that all results are normal. If error was detected, contact your local distributor or Kyoto Kagaku with the error code.

Proble	m detecte Conn		Normal		
	Spea	ker Device #1 :	Normal		
Error co	ode <mark>00000</mark>	0			




Do not operate the control PC while the error indicator system is working.

Starting up the software

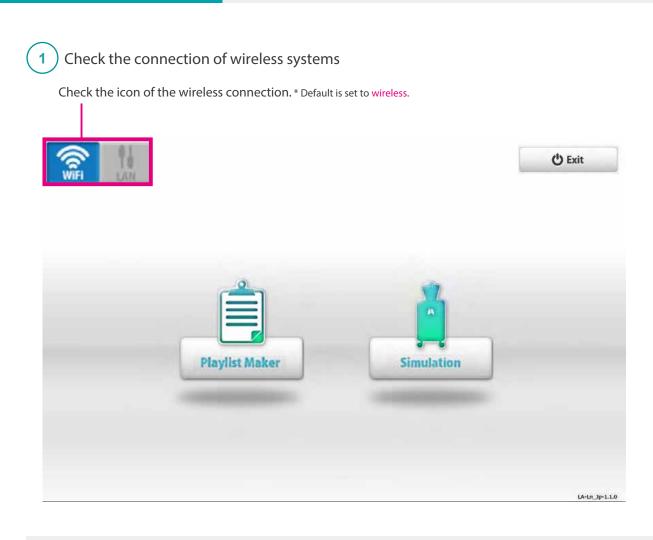



The softwares include help menu for how to use the simulator. Tap the help menu for more details which are not described in this manual.

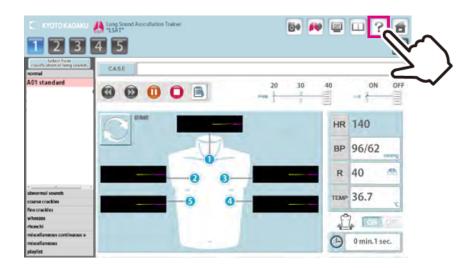

Starting up the software Selecting unit



Start up simulation software

From top menu, select "Pediatric LSAT Simulation" or "Playlist Maker".



Softwares



Pediatric LSAT Simulation Software

All functions of Pediatric LSAT are operated by this software.



3


Pediatric LSAT Playlist Maker

"Playlist" of cases can be created. To create a playlist,

- 1) Use the Playlist Maker. Select cases, set their sequence and running time for each, then name and save the list.
- 2) Save a session as a playlist on Pediatric LSAT Simulation software. In the Playlist maker, data of recorded playlists can be edited and modified.

Select units to operate

Tap the units to operate and then tap "OK."

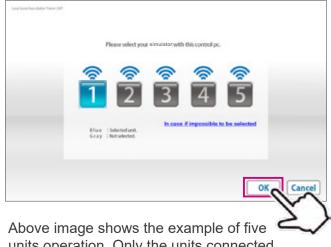

Above image shows the example of five units operation. Only the units connected to the PC appear on the screen. The button color indicates the status of each unit.




"Blue": The units selected by this PC.

"Green" : The units already connected by another PC and not available to this PC.




"Gray" : The units unselected.




Inactive



Error indication has been completed, the simulation software is ready to begin.

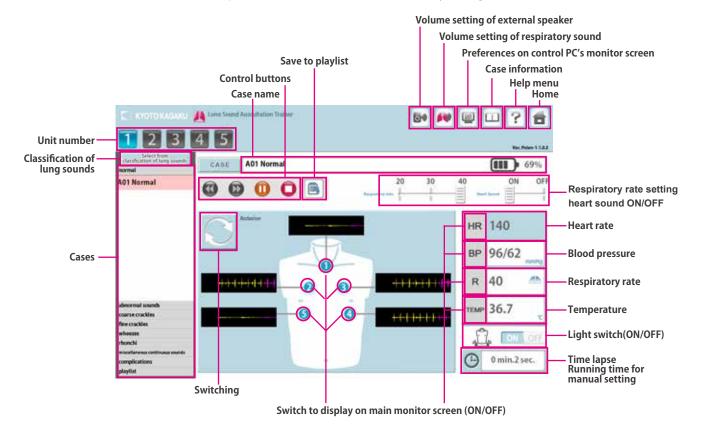

2) Playlist Maker

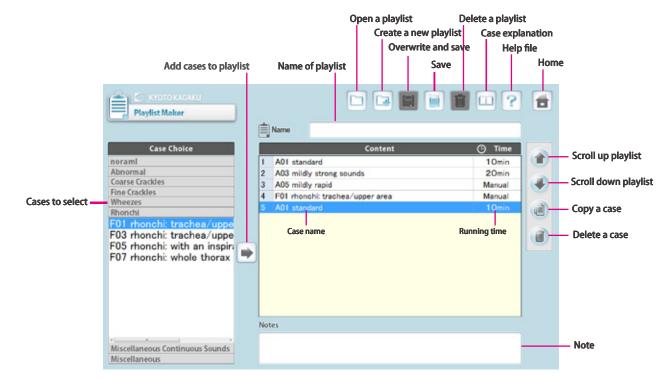

Multi-unit operation

Multi-unit operation


Up to 5 units can be operated by one control PC.

Setting process varies between unison operations and multiple case operations. For details see incorporated HELP menu by tapping on the rank on the top right of the screen.

One simulator unit (torso) can be selected by only one control PC at a time. The connections are established in the order of selecting the units.

IMPORTANT

For example, while units #3 and #5 are selected by control **PC B**, the control **PC A** cannot select these units. To connect them to control **PC A**, these units need to be unselected by control **PC B**.

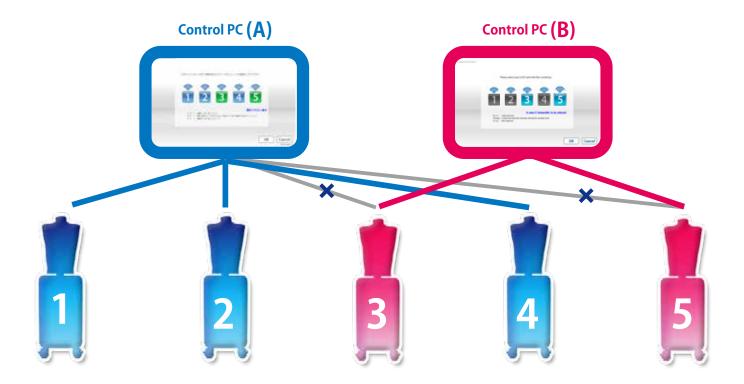


After Training


Exiting the software Turning off the control system's main power

) Exit software

1

Tap on the "Home" icon at the right top. "Do you want to exit?" message appears, select "Yes."

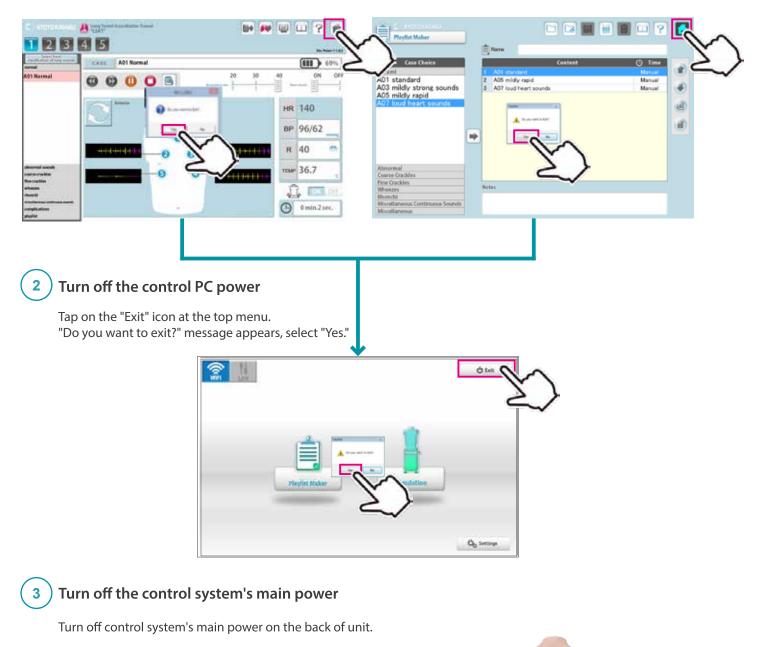

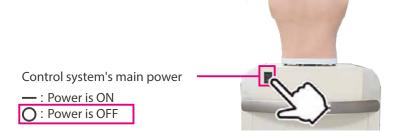

Trouble shooting

Trouble shooting list

Cases	Causes	Solutions				
Unable to connect with wireless	Network interference occurred.	\rightarrow Case: Unable to Boot The Main Unit (\rightarrow P.19)				
or unstable connection	There are physical obstructions for wireless connection or control PC is too far from the unit.	Clear the obstructions or close the control PC to the unit.				
	Power cable of the unit is not connected.	Connect the power cable.				
Unable to boot the main unit with	The main power of the unit is off.	Turn on the main power of the unit.				
wireless connection	Network interference occurred.	Consultable to Doot The Main Heit (), D (0)				
	Others	\rightarrow Case: Unable to Boot The Main Unit (\rightarrow P.19)				
	The control PC does not correspond to the unit.	Use the control PC corresponding to the unit.				
Unable to select the units which	The main power of the unit is off	Turn on the main power of the unit.				
liked to boot	Power cable of the unit is not connected.	Connect the power cable.				
	Network interference occurred.	-> Case: Unable to Select The Units (> D.20)				
	Others	\rightarrow Case: Unable to Select The Units (\rightarrow P.20)				
The session automatically shuts down with the message of "Connection Error", and then the connection becomes unavailable.	Network interference occurred.	→ Case: The Error Occurs During The Session (→ P.21)				
Unable to hear the respiratory	Volume setting of the respiratory sound is "0"	→ Volume Setting of The Respiratory Sound				
sound from the manikin	Speaker connection may have problems.	→ Contact Us				
Unable to hear the heart sound	Volume setting of the heart sound is "0"	→ Volume Setting of The Heart Sound				
from the manikin	Speaker connection may have problems.	\rightarrow Contact Us				
Unable to hear the sound from	Volume setting of the external speaker is "0"	→ Volume Setting of The External Speaker's Sound				
the external speaker	Speaker connection may have problems.	→ Contact Us				

Trouble shooting


Unable to boot the main unit

Attention

For the multi-unit operation, be sure the control PC's own main unit is turned on. The control PC is unable to operate when its own main unit is turned off.

Case:

The screen shows the sign below repetitively and does not work despite several trials.

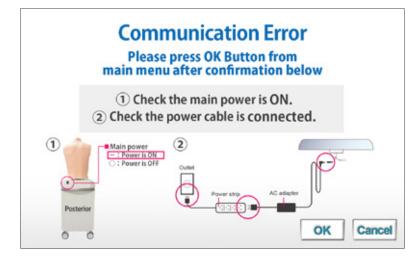


Cause and **Solution** 1:

- 1. The main units are not connected to power source.
 - \rightarrow Connect the cable to power source and turn on the main unit.
- 2. The main units are not turned on.
 - \rightarrow Turn on the main units.
- 3. Interference from other wireless network
 - \rightarrow Follow the solution 2 below.

Solution 2:

Tap "Cancel" to go back to the top page and try with LAN connection mode.

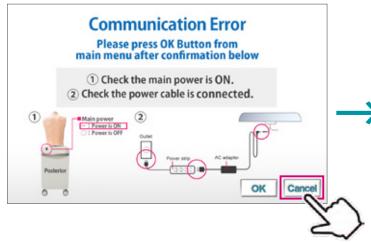

\mathcal{L}		(ð fait
Playlist Maker	Simulation	
 _	-	1844.9

How to switch to LAN connection mode : P.22

Trouble shooting

Unable to select the units

Attention

For the multi-unit operation, be sure the control PC's own main unit is turned on. The control PC is unable to operate when its own main unit is turned off.

Case:

Units are unable to be selected.

Catalog Peterstrongent Please select your LSAT unit with this control pc. Image: Imag	 The connection indicator is gray on the unit.
OK Cancel	

Cause and solution:

- 1. The main units are not connected to power source.
 - \rightarrow Connect the cable to power source and turn on the main unit.
- 2. The main units are not turned on.
 - \rightarrow Turn on the main units.
- 3. Interference from other wireless network
 - \rightarrow Follow the solution 2 below.

Solution 2:

Tap "Cancel" to go back to the top page and try LAN connection mode.





How to switch to LAN connection mode: P.22

Error occurs during the session

Case:

The software is automatically closed with the error message below.




Cause:

Wireless network is confused around the models.

Solution:

Try LAN connection mode.

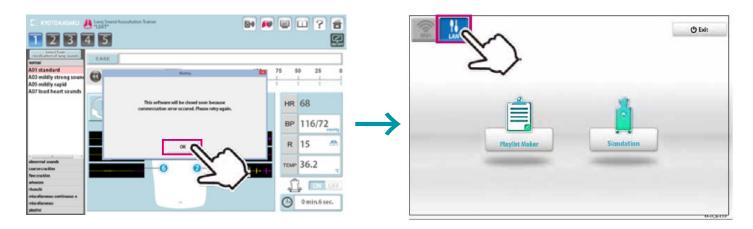


Error occurs during the session

1) Tap the network icon on left upper display to switch the connection mode.



2 Connect the control PC to the LAN cable from the main unit .

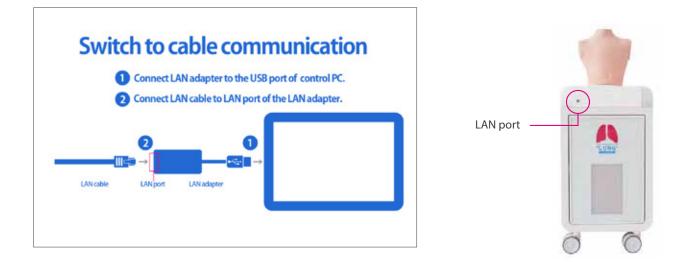

Attention

Regarding multi-unit operation with the LAN connection mode, check the attached paper.

Pediatric Lung Ausculation Trainer

Caution

Do not mark on the model and its components with a pen or leave printed materials in contact with the model surface. Ink marks on the model are not removable.

MW57 Pediatric Lung Sound Auscultation Trainer

Worldwide Inquiries and Orders

Kyoto Kagaku Head Office and Factories: TEL: +81-75-605-2510 FAX: +81-75-605-2519 15 Kitanekoya-cho, Fushimi-ku, Kyoto, 612-8388, JAPAN

USA, Canada, and South America

Kyoto Kagaku America Inc. TEL: 1-310-325-8860 FAX: 1-310-325-8867 3109 Lomita Boulevard, Torrance, CA 90505-5108, USA

Europe, Russia & Africa

Kyoto Kagaku Europe GmbH.

TEL: +49-69-5060-28160

De-Saint-Exupery-Str.10, 60549 Frankfurt, Germany

Greater China Area

Hong Kong Representative Office

TEL: +86-852-3978-1365 FAX: +86-852-3978-1199

Level 23, One Island East, 18 Westlands Road, Island East, Hong Kong

KYOTO KAGAKU co., ltd

URL: http://www.kyotokagaku.com e-mail: rw-kyoto@kyotokagaku.co.jp

The contents of the instruction manual are subject to change without prior notice.

No part of this instruction manual may be reproduced or transmitted in any form without permission from the manufacturer. Please contact manufacturer for extra copies of this manual which may contain important updates and revisions. Please contact manufacturer with any discrepancies, typos, or mistakes in this manual or product feedback. Your cooperation is

Please contact manufacturer with any discrepancies, typos, or mistakes in this manual or product feedback. Your cooperation is greatly appreciated.