




**Caution** Don't mark on the phantom with pen or leave printed materials contacted on its surface. Ink marks on the phantom will be irremovable.

### Simulated lesions in liver, pancreas, kidney, spleen, gallbladder

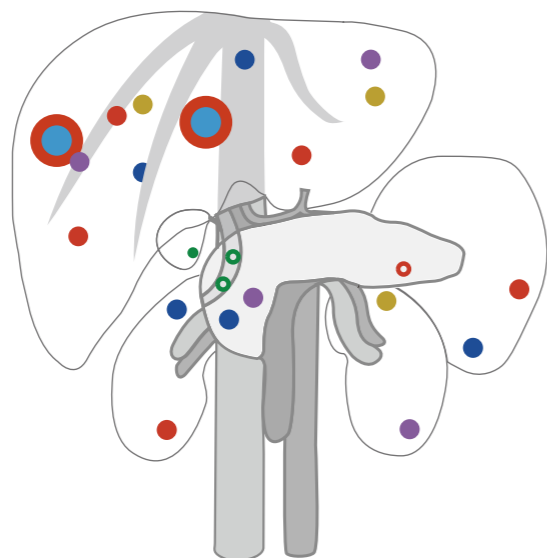

#### Anatomy

lung / kidneys (right and left) / gallbladder / aorta/ liver (portal vein, bile duct, hepatic artery, hepatic vein) / spleen / pancreas (pancreatic duct) / inferior aorta / spine / ribs

#### Abnormal lesions

liver / gallbladder / pancreas / spleen / kidney

- Liver lesions (cysts, solids)
- Gallbladder and bile duct stones
- Pancreatic tumors
- Spleen lesions
- Left and right kidney lesions

[Embedded Targets]		Liver	Gallbladder	Pancreas	Spleen	Kidney(R)	Kidney(L)
		HU70	HU20	HU30	HU50	HU30	HU30
anechoic	● Φ10mm	3			1	1	
	○ Φ3mm	HU50		1	HU10	HU10	
hypoechoic	● Φ10mm	2					1
		HU50					HU10
medium echo	● Φ10mm	2		1			1
		HU90		HU10			HU10
hyperechoic	● Φ10mm	2		1	1	1	
		HU90		HU10	HU10	HU10	
double echo lesion inside: hyperechoic outside: anechoic	● Φ20mm	2					
		HU90					
gallstones	● Φ5mm		1				
	○ Φ3mm		HU170	2			
				HU170			

The contents of this manual are subject to change without prior notice.  
 No part of this instruction manual may be reproduced or transmitted in any form without permission from the manufacturer.  
 Please contact manufacturer for extra copies of this manual which may contain important updates and revisions.  
 Please contact manufacturer with any discrepancies, typos, or mistakes in this manual or product feedback.  
 Your cooperation is greatly appreciated.



URL: <http://www.kyotokagaku.com> e-mail: [rw-kyoto@kyotokagaku.co.jp](mailto:rw-kyoto@kyotokagaku.co.jp)

#### Main Office and Factory

15 KitaneKoya-cho Fushimi-ku Kyoto 612-8388, Japan  
 Telephone : 81-75-605-2510  
 Facsimile : 81-75-605-2519


#### KyotoKagaku America Inc.

USA, Canada, and South America  
 3109 Lomita Boulevard, Torrance, CA 90505, USA  
 Telephone : 1-310-325-8860  
 Facsimile : 1-310-325-8867

#### Caution:

Don't mark on the phantom with pen or leave printed materials contacted on its surface. Ink marks on the phantom will be irremovable.

## US-22 Dual Modality Human Abdomen Phantom

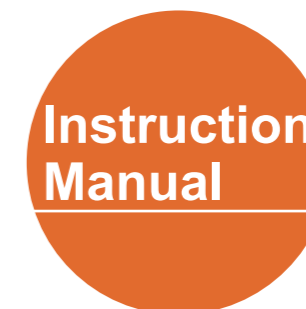

### Contents

- Please read before training
  - General information ..... P. 1
- Preparation
  - 1. Before training ..... P. 2
- Training
  - 2. Training session ..... P. 2
  - 3. After training ..... P. 2



#### ● This phantom is a comprehensive diagnostic imaging training phantom that uses fusion imaging.

This phantom is designed to confirm lesions noted on CT as well as ultrasound.  
 ※For effective training, use ultrasound devices that is under appropriate control.


This phantom is designed for a step-by-step learning process from the basic of ultrasound screening to organ-specific screening procedures and screening for intra-organ lesions.  
 Please do NOT use this phantom outside of its purposes.

#### ● Features

- The new material is compatible with CT and ultrasound.
- The phantom includes nearly full-scale and accurate lungs, aorta, gallbladder, inferior vena cava, liver (portal vein, bile duct, hepatic artery, hepatic vein), kidneys (left and right), pancreas (pancreatic duct), spleen, and ribs.  
 Cysts, stones, tumors and other lesions with different sizes, echo, CT values are also included, which allows simultaneous anatomic understanding and training in simple screening.  
 ※Biopsy and other punctures cannot be performed.

Set includes

Before your first use, please ensure that you have all components listed below.

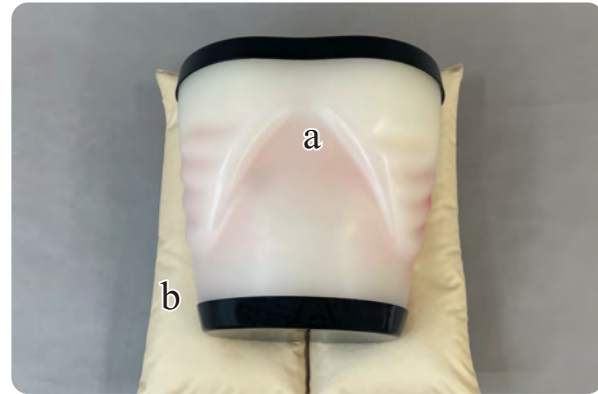

- Set includes
- a. Dual modality abdominal phantom ..... 1  
the liver (segmental anatomy, portal and hepatic venous systems, hepatic circumflex and ductus venosus), biliary tract (gallbladder, cystic duct, intrahepatic and extrahepatic bile ducts), pancreas (pancreatic duct), spleen, kidneys, detailed vascular structures (aorta, vena cava, celiac artery and its branches, portal vein and its branches, superior mesenteric vessels, renal vessels, etc)
- b. Positioning pillow ..... 1
- c. Talcum Powder ..... 1
- d. sample CT images (DVD) ..... 1
- e. Instruction Manual (this leaflet) ..... 1

The setting of supine position and the lateral position is possible using a positioning pillow.



⚠ DOs and DON'T s

**DO s**

- Handle with care
- The materials for the phantom are special composition of soft resin. Please handle with care at all times.
- Cleaning and care
- Please clean the phantom completely every time after you finish the training.
- The remaining ultrasound gel may deteriorate the phantom.
- Keep the training set at room temperature, away from heat, moisture and direct sunlight.

**DON'Ts**

- Never wipe the phantom with thinner or organic solvent.
- Don't mark on the phantom with pen or leave printed materials contacted on their surface. Ink marks on the surface will be irremovable.

Please note: The color of the phantom may change over time, though, please be assured that this is not deterioration of the material and the ultrasonic features of the phantom stay unaffected.

This phantom has a thin layer of coating for protective purposes which may cause minor wrinkling. However, it has no effect on the ultrasound image.



Please watch the following movie about handling precautions of ultrasound phantoms.

<https://www.youtube.com/watch?v=D3VcaUYcPAY>

1 Before training



1. Set the phantom on the positioning pillows.



2. Apply ultrasound gel on the phantom body.

2 Training session




1. The phantom can be scanned with actual ultrasound devices.  
\* The map of simulated targets is on the backside of this manual.

Examples of ultrasound images



Duplication lesion

Low echo target

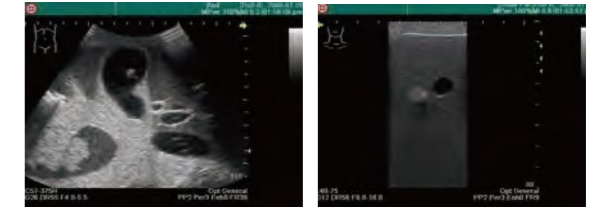

Gallstone

High and non echo targets

3 After training



Wipe the remaining gel completely with wet cloth. If remaining gel gets dried up on the body, it will be irremovable.